
LABORATORY ELECTRODES

6/11



6103 GLENMONT • HOUSTON, TEXAS • 77081 800/522*7920 • FAX713/772-4671 • 713/772-6641 www.VL-PC.com

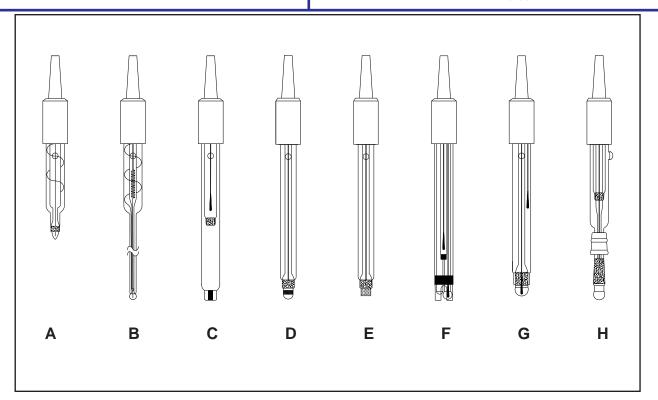


- **A** Combination pH spear tip with refillable reference used with semi-solid samples such as meats, cheeses and polymers.
- **B** Combination pH dual diameter body with refillable reference used for measurements in test tubes and other small containers.
- **C** Mono reference electrode can be either AgCl or Calomel with refillable reference for use with mono measuring electrodes.
- **D** Combination ORP with platinum band and refillable reference
- **E** Combination Ion Selective electrode silver/sulfide with refillable reference.
- **F** Combination pH with temperature sensor built into an epoxy body used with bench and portable meters.
- **G** Combination pH with ruggedized tip and refillable reference used in environments where breakage is possible.
- **H** Combination pH with sleeve reference and refillable reference used in samples that quickly clog standard reference junctions.

Additional electrode styles, buffer solutions, wiring adapters and meters are available. Consult the factory for options and additional product information. Call 713/772-6641 or 800/522-7920

Email: info@VL-PC.com www.VL-PC.com

VAN LONDON - PHOENIX CO. LABORATORY/TITRATION/ION SELECTIVE ELECTRODE PART NUMBER GUIDE #2

Rev. 04/14/05
[W:\Main\PM70\PNGuide]

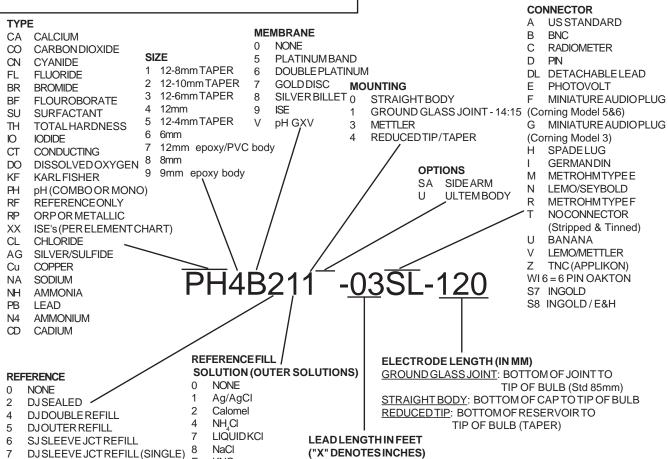

* SPR - SOLID POLYMER REFERENCE

KNO₂

SPR-KCI



DJTFE SLEEVE JCT REFILL (SINGLE)

DJPHREE FLOW OUTER REFILL


8

q

Т

POLAROGRAPHIC

GALVANIC

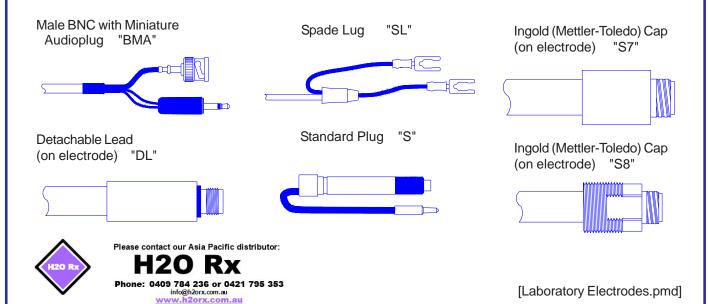

3 FOOT IS STANDARD